

Variable Angle Screw

Specification	
D	L
Φ4.0	11
Φ4.0	12
Φ4.0	13
Φ4.0	14
Φ4.0	15
Φ4.0	16
Φ4.0	17
Φ4.0	18
Φ4.0	19
Φ4.5	11
Φ4.5	12
Φ4.5	13
Φ4.5	14
Φ4.5	15
Φ4.5	16
Φ4.5	17
Φ4.5	18
Φ4.5	19
Φ4.5	20
Φ4.5	21



Anterior Cervical Plate

Specification	
The number of holes	L
4	21
4	23
4	25
4	27.5
4	30
4	32.5
4	35
6	35
6	37.5
6	40
6	42.5
6	45
6	47.5
6	50
8	52.5
8	55
8	57.5
8	60
8	62.5
8	65
8	67.5
8	70
8	72.5
10	75
10	77.5
10	80
10	82.5
10	85
10	87.5
10	90
12	95
12	100




Fixed Angle Screw

Specification	
D	L
Φ4.0	11
Φ4.0	12
Φ4.0	13
Φ4.0	14
Φ4.0	15
Φ4.0	16
Φ4.0	17
Φ4.0	18
Φ4.0	19
Φ4.5	11
Φ4.5	12
Φ4.5	13
Φ4.5	14
Φ4.5	15
Φ4.5	16
Φ4.5	17
Φ4.5	18
Φ4.5	19
Φ4.5	21
Φ4.5	20

Features

- Plate thickness of 2.1 mm and low profile reduce the potential esophageal irritation
- Easy intraoperative observation of bone graft location
- Auto-locking mechanism avoids screw pull-out and enables stability
- Fixed and variable angle screws for better adaptability
- Streamlined procedures help time-saving surgery
- Our products are manufactured using one or more of the following materials: commercially pure titanium (ISP 5832-2, ASTM F67), Ti6Al4V alloy (ISO 5832-3, ASTM F1472)

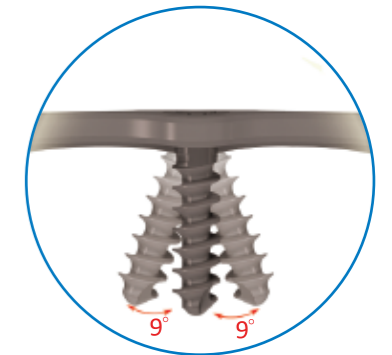

Indications

Cervical spine (C2-C7) instabilities associated with:

- Fractures / dislocations
- Degenerative diseases
- Tumors
- Congenital diseases

